


dB Ref Level : 0 dB
Ref Offset : 0.0 dB

● Detector : Sample
Trigger Mode : Free Run
Trace : Clear / Write

RBW : 1 MHz
VBW : 1 MHz
SWT : 100 ms

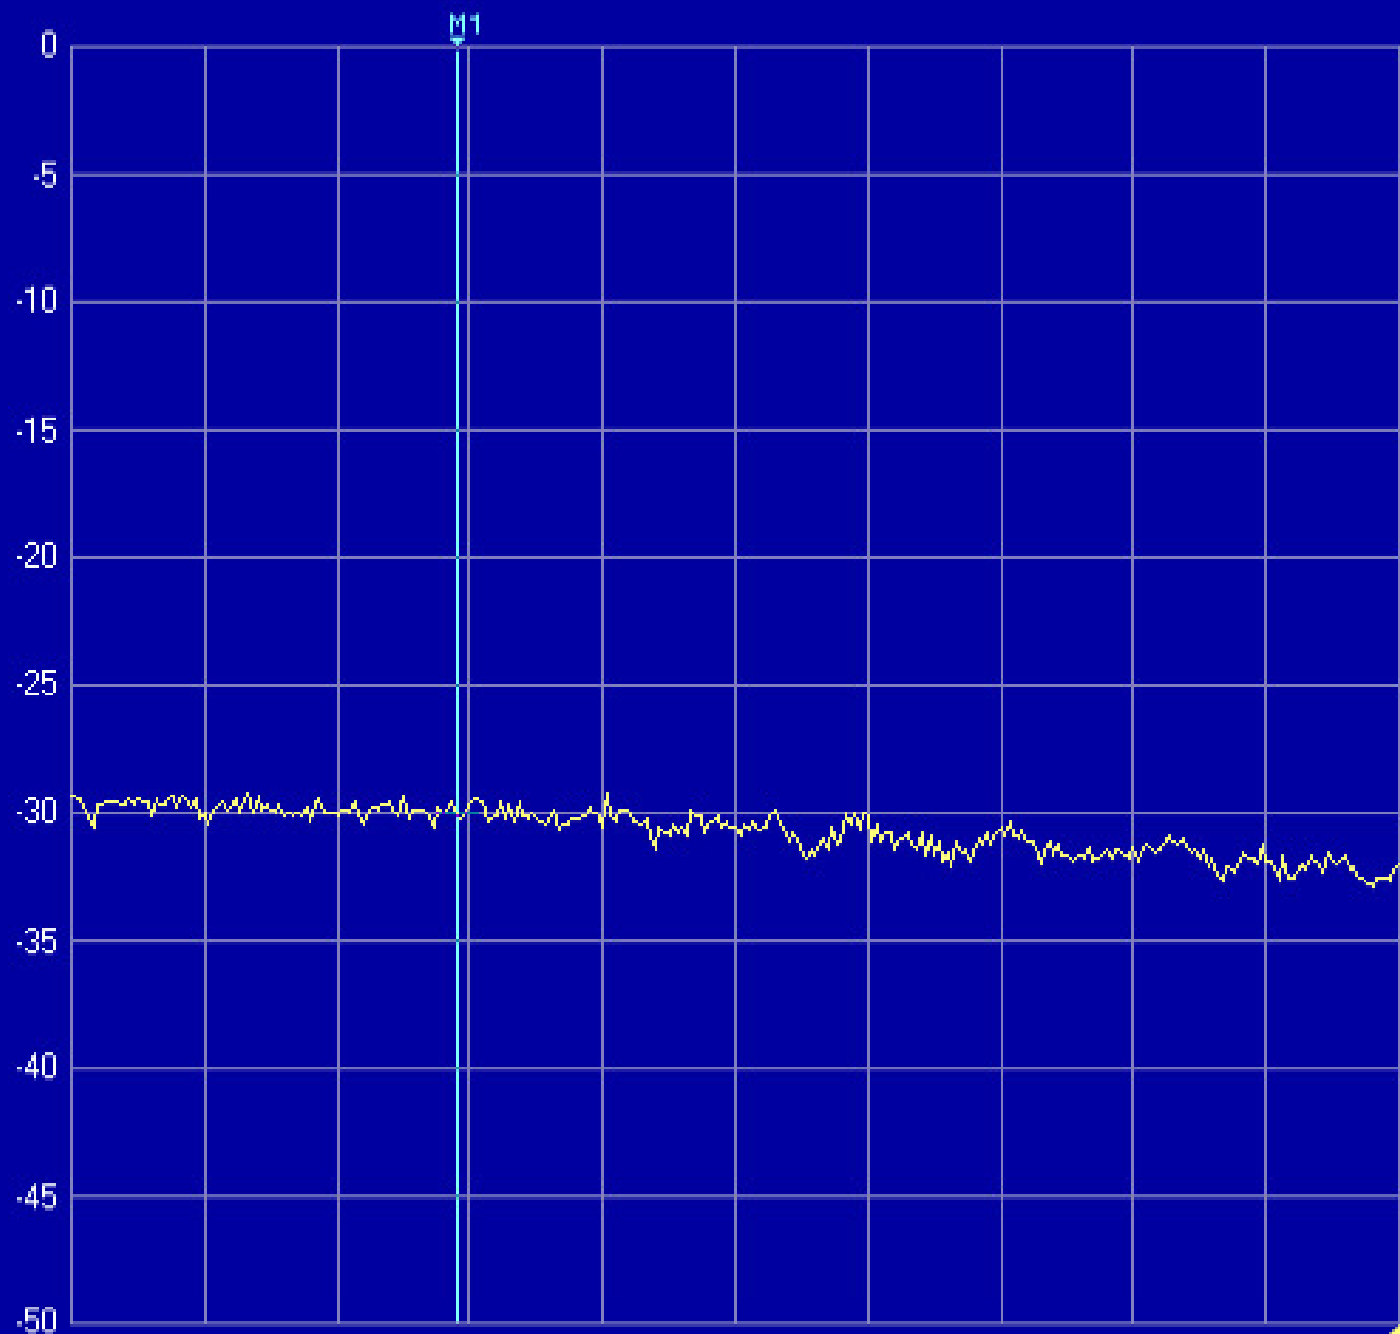

Trace	
File Name	---
Name	Transmission (scalar)
Ref Level	: 0 dB
Range	: 5 dB/div
Bw/	: -- Hz
Result	---
Averaging	---

Status	
VSWR-Bridge	: No Bridge
Center Frequency	: 750 MHz
Span	: 1.5 GHz
Ref Offset	: 0.0 dB
Trace Offset	: 0.0 dB
RF Attenuator	: 0 dB
Preamplifier	: Off
Dynamic Range	: Low Distortion
RF Input	: 50 Ohm
RBW	: 1 MHz
VBW	: 1 MHz
SWT	: 100 ms
Trace Mode	: Clear / write
Detector	: Sample
Trigger Mode	: Free Run
Trigger Level	: ---
Trigger Delay	: ---
Calibration Kit	: FSH CalKit
Offset Length	: 0 mm
Upper Limit	: ---
Lower Limit	: ---
External Reference	: Disabled
Date	: 04/05/2018
Time	: 15:06:43
Instrument	: FSH13 - 102668
Operator	: ---

Markers	
M1 :	435 MHz : -30.01 dB

Transmission (scalar)

Start Frequency : 0 Hz
Center Frequency : 750 MHz

Stop Frequency : 1.5 GHz
Span : 1.5 GHz